

# Raman Monitoring Systems (RAMS™)



- **High throughput VPH grating spectrograph**
- **Rack mountable housing**
- **Can monitor up to 6 different probes simultaneously**
- **Each probe is connected to its own laser**

Our Raman monitoring systems (RAMS™) is a single or multi-probe input Raman instrument that is capable of real-time, simultaneous measurements of multiple fiber optic probes (up to 6 channels).


- **A high throughput volume phase holographic grating spectrograph** with a **2-dimensional TE-cooled CCD detector** is employed for detection.
- **A linear fiber optic array bundle mounted parallel to the slit direction** is coupled into the spectrograph entrance aperture to allow multiple probe coupling.
- **Multiple tracks are setup with the 2-dimensional CCD chip corresponding** to the positions of the individual fiber in the imaged linear fiber optic array.
- The multiple tracks allow the implementation of **multiple probe simultaneous measurements.**
- For the RAMS™ multichannel version, **each channel has a dedicated laser for Raman excitation.**

## FEATURES


- The RAMS™ instrument can be controlled with our **SpectraSoft data acquisition software.**
- With the **chemometrics plug-in software, SpectraChem, implemented with SpectraSoft,** the RAMS™ instrument can be used for on-line process monitoring applications.
- Different types of probes are available for use with the RAMS™ instruments including **high pressure, vacuum and high temperature** Raman immersion probes.

## Specifications

<b>Excitation Wavelength</b>	532 nm, 671 nm, and 785 nm.
<b>Raman Shift Range</b>	532 nm: 150-4100 $\text{cm}^{-1}$ ; 671 nm: 150-4000 $\text{cm}^{-1}$ ; 785 nm: 150-3000 $\text{cm}^{-1}$
<b>Laser Power</b>	200 mW
<b>Fiber Input</b>	100 $\mu\text{m}$ with FC connector standard, other core sizes and SMA connector available
<b>Spectrograph</b>	High throughput VPH grating with F2 optics
<b>Detector</b>	Andor IVAC CCD, 1650 x 200 active pixels (16 x 16 $\mu\text{m}$ pixel size)
<b>CCD TE Cooling</b>	-60 $^{\circ}\text{C}$ at ambient (25 $^{\circ}\text{C}$ )
<b>Power Input</b>	90-264 VAC
<b>Communication</b>	USB
<b>Software</b>	SpectraSoft data acquisition software included, SpectraChem plug in software for process applications also available
<b>Computer and Operating Software Requirements</b>	Windows 7 64-bit or later, Intel Core i3 or comparable processor, 4GB of memory & 100MB of free hard drive space
<b>Instrument Housing</b>	19" Rackmount housing, 4U for single channel and 6U for multiple channels
<b>Coupling System</b>	FC Connector
<b>Dimensions &amp; Weight</b>	6.97"x19.00"x10.43", 21 lbs
<b>Part Number</b>	RAMS-532, RAMS-671, RAMS-785

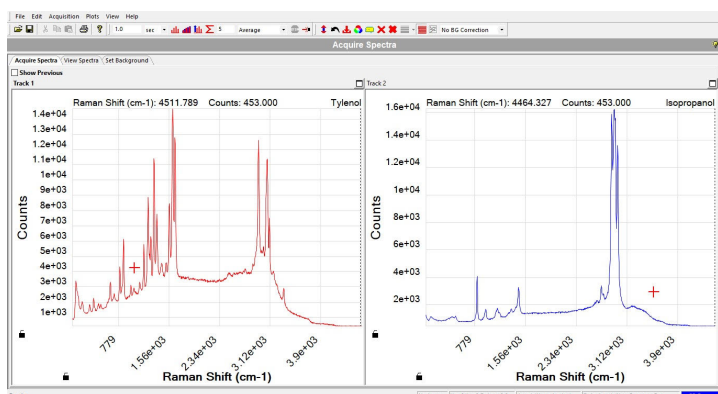

Simultaneous analysis of 2 samples with separate Raman probes

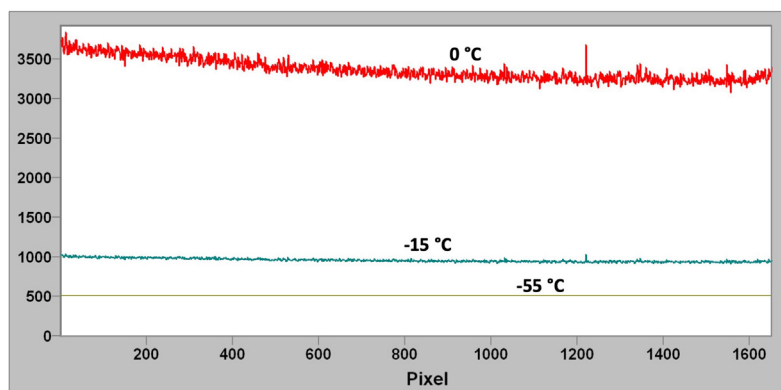

Dark current at different CCD cooling temperatures, 1 s integration